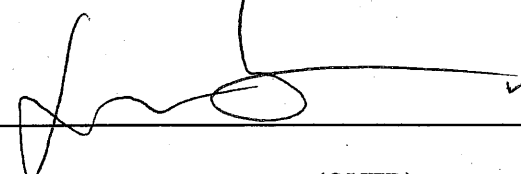


DEC 02 2008
VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program


		DataMaster cdm S/N <u>130569</u> ✓	
Supervisor/Operator Performing the Verification Procedure:			
Name <u>John Hodges</u>		ID # <u>2999</u>	Date <u>11/28/2008</u> ✓
A	Agency <u>Cordova Police Department</u>		Phone # <u>424-6100</u>
Instrument Location <u>Cordova Police Department</u> ✓			
B			
Alco S/N <u>X124656</u> ✓		Target Value <u>0.076</u> ✓	High Pressure <u>200psi</u>
Alco Test Value Average <u>0.077</u> ✓		<u>0.077</u> ✓	
1st Alco		2nd Alco	
Signature 		CCB 12/5/08	

Under the Alaska Rules of Evidence, I certify (OVER)


(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, John Hodges, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

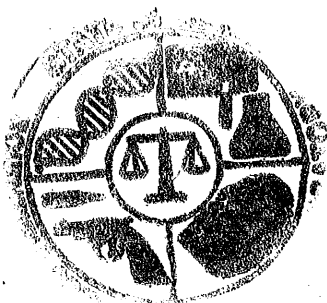

Signed and sealed,



Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

12/5/08
Date

VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program

DataMaster cdm S/N

130569 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130569

NOVEMBER 28, 2008

OPERATOR'S NAME:

HODGES, JOHN

OPERATOR'S NUMBER: 2999

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

X

O.L. #: X

DEPT/AGENCY: CDV1

CASE/REPORT: X

TEST TYPE: V

ALCO TARGET VALUE: .076 ✓

ALCO S/N: X124656

--- BREATH ANALYSIS ---

.076 ADJUSTED FOR 29.23 in

ALCO TARGET .074 00:38

BLANK TEST .000 00:39

INTERNAL STANDARD VERIFIED 00:39

ALCO TV 29.23 in .077 ✓ 00:39

BLANK TEST .000 00:40

SUBJECT SAMPLE .000 00:41

BLANK TEST .000 00:42

ALCO TV 29.23 in .077 ✓ 00:42

BLANK TEST .000 00:43

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130569

NOVEMBER 28, 2008 ✓

TIME 00:44

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 45c

BREATH TUBE: 40c

BAROMETER: 29.25 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJ
KLMNOPQRSTUVWXYZ[\] ^ _ `abcde-fghijklmno
pqrstuvwxyz{|}~